

The most reliable LC-EC
applications for
Antibiotics analysis

Aminoglycosides

Amikacin
Framycetin Sulphate
Gentamicin Sulphate
Kanamycin Sulphate
Lincomycin
Neomycin
Spectinomycin
Tobramycin

Macrolide antibiotics

Azithromycin
Azaerythromycin
Clarithromycin
Erythromycin
Roxithromycin

Tobramycin in Pharmaceutical Preparations

-
- **European Pharmacopoeia 6.0 (2008) used as basis for this application**
 - **FlexCell with exchangeable gold electrode**
 - **Analysis of main substituent and impurities**
 - **Reproducible & robust**
-

Summary

The European Pharmacopoeia describes a method for the analysis of Tobramycin and its impurities based on LC-PAD [3]. The ALEXYS analyzer based on the Antibiotics LC base system with post-column addition kit is a dedicated solution for the analysis of aminoglycoside antibiotics using a silica-based C18 column.

In this application note results are shown for the analysis of Tobramycin and its impurities using the ALEXYS analyzer.



Introduction

Tobramycin belongs to the group of the aminoglycoside antibiotics. Like the other aminoglycosides, it binds to bacterial ribosomes and causes non-functional proteins to accumulate within the cell leading to cell death. It is often effective against bacterial strains that prove resistant to other aminoglycosides like gentamicin. The production is mainly achieved by fermentation resulting in several minor by-products.

The analysis of the byproduct contribution in bulk tobramycin and preparations is important as to insight in stability, quality control and authenticity. A number of qualitative and quantitative methods has been published so far [1] but the focus is mainly on tobramycin and not on the by-products. Because of the presence of sugar groups in both tobramycin and by-products LC with pulsed amperometric detection (PAD) is a highly selective and sensitive analytical tool [2].

Method

The ALEXYS analyzer (see figure 1) is a versatile solution, it contains all LC hardware and the analytical column for the analysis of several aminoglycosides including Neomycin, Tobramycin and Spectinomycin. The Analyzer is equipped with a second pump for the post-column addition of NaOH. Addition of NaOH is necessary to make the mobile phase strongly alkaline ($\text{pH} > 12$), in order to allow PAD detection of the aminoglycosides using an Au electrode [2]. The mobile phase was prepared as described in the European Pharmacopoeia monograph [3].

Table 1

LC-EC Conditions	
HPLC*	ALEXYS Analyzer for Tobramycin
Flow rate	1 mL/min, post-column: 0.6 mL/min
Cell	FlexCell™ with Au WE and HyREF™
Sample	20 µL
Mobile phase	52 g/L Na ₂ SO ₄ , 1.5 g/L OSA, 3 mL/L THF stabilized, 10 mmol/L KH ₂ PO ₄ , pH 3
Addition	0.76 mol/L NaOH post-column
Temperature	45 °C for column, mixing and flow cell
E-cell	E1, E2, E3: 0.1, 0.75, -0.15 V ts, t1, t2, t3: 0.1, 0.32, 0.2, 0.4 s
I-cell	ca. 2 µA

* Note that the presented data are obtained with an older version of the ALEXYS LC system than shown in fig 1.



Figure 1: ALEXYS analyzer for Tobramycin.



Results

In an example chromatogram is shown of a 20 μL injection of 100 $\mu\text{g/mL}$ Tobramycin dissolved in mobile phase. The chromatogram is zoomed in on the baseline to show the impurities (Kanamycin B, Neamine). The impurity Kanamycin B and Tobramycin are sufficiently separated with a resolution of 3.07.

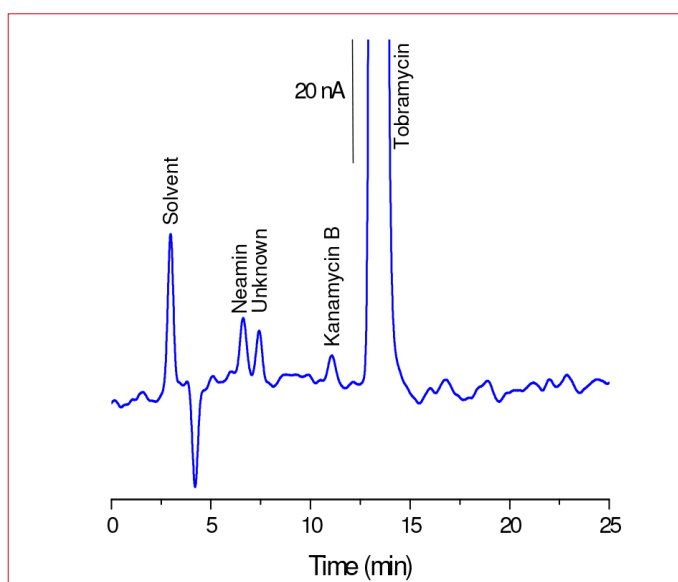


Figure 2: Tobramycin sample (100 $\mu\text{g/mL}$, 20 μL injected). The peak height of the Tobramycin peak is 2.32 μA . Impurities as percentage % of the main peak are: Neamin 0.38%, unknown 0.29%, Kanamycin B 0.19%.

The EP requires a resolution > 3 . In the EP monograph the concentration of octane sulphonic acid in the mobile phase is designated as a variable to optimize the resolution between Kanamycin B and the principal peak (Tobramycin). This parameter can be used to increase the resolution if necessary.

Another EP system suitability requirement is the signal-to-noise ratio of the principle peak of a 20 μL injection of reference standard B (2.5 $\mu\text{g/mL}$ Tobramycin CRS solution). The S/N ratio of the principle peak in that case should be larger than 10. The signal-to-noise ratio for the principle peak using the ALEXYS analyzer was estimated to be around 15 under the specified conditions (estimation based on the noise and peak height of the principle peak in the chromatogram shown in figure 2, the value for peak height was divided by 40 to reflect a concentration of 2.5 $\mu\text{g/mL}$ Tobramycin).

Conclusion

The ALEXYS® analyzer is a suitable solution for the analysis of Tobramycin and its impurities in bulk drugs.



Tobramycin in Pharmaceutical Preparations

References

1. David A. Stead, "Current methodologies for the analysis of aminoglycosides", J. Chromatogr. B, 747 (2000) 69–93
2. W.R. LaCourse, "Pulsed Electrochemical Detection in High Performance Liquid Chromatography", John Wiley & Sons, New York, 1ed, 1997.
3. "Tobramycin", European Pharmacopoeia, 6.0, (2008) 3085-3086

Ordering information

Recommended ALEXYS analyzer + parts	
180.0058W	ALEXYS Antibiotics base system - Isocratic
180.0605EP	Post Column Kit EP
102.4325EP	Flexcell Au HyREF with stainless steel AUX
250.1045	Flattening/polishing kit for metal WE
184.0209	Glass bottle assembly, 1L, Helium
Column	
00G-4252-E0*	Luna® C18 column, 250 x 4.6 mm ID, 5 µm

*) The column is manufactured and sold by Phenomenex Inc., Torrance, California, USA. Luna is a registered trademark of Phenomenex Inc.

For research purpose only. The information shown in this communication is solely to demonstrate the applicability of the ALEXYS system. The actual performance may be affected by factors beyond Antec's control. Specifications mentioned in this application note are subject to change without further notice.

Antec Scientific (USA)
info@AntecScientific.com
www.AntecScientific.com
T 888 572 0012

Antec Scientific (worldwide)
info@AntecScientific.com
www.AntecScientific.com
T +31 71 5813333

