


On the backside important installation information is provided for the parts marked with a caution sign. Please read this instructions before starting.



#### Legend of LC connectors

■	250.1550 Ferrule Tefzel, 1/8", flangeless
■	250.1552 Nut PEEK, 1/8", flangeless, 1/4-28
■	250.1566 Ferrule CTFE, 1/8", collapsible
■	250.1568 Nut PEEK, 1/8", hex, 5/16-24
■	250.1591 Ferrule SS, 1/32", Valco
■	250.1590 Nut SS, 1/32", Valco, 10-32
■	250.1558 Ferrule SS, 1/16", Valco
■	250.1560 Nut SS, 1/16", Valco, 10-32
■	250.1572 Fingertight PEEK, hex, 10-32
■	250.1571 Fingertight PCTFE, 10-32

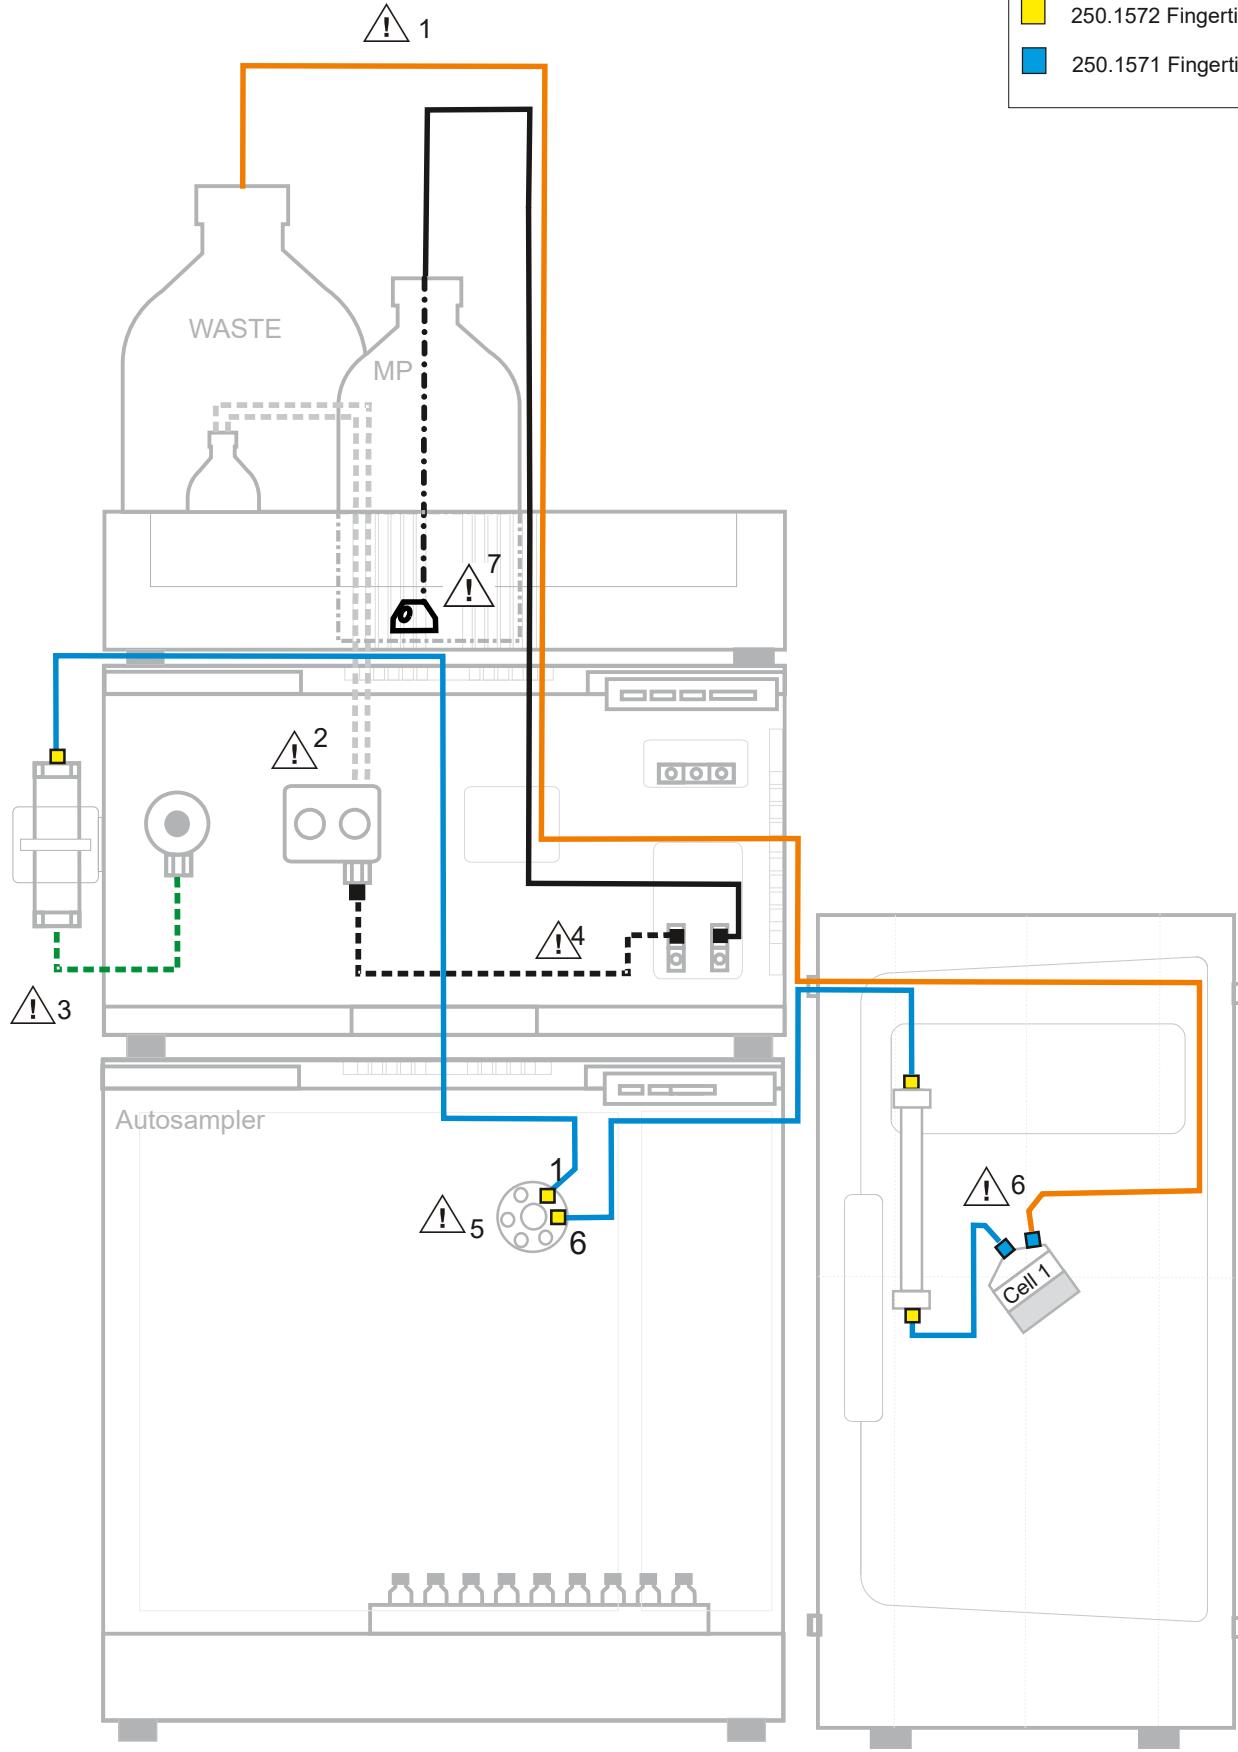

LC equipments should be used by trained laboratory personnel only. Use proper eye and skin protection when working with solvents under high pressures. Additional safety requirements or protection may be necessary depending on the chemicals used with this equipment.



## IMPORTANT INSTALLATION INFORMATION

Read the LC connection kit install guide (p/n 180.7001W), before installation of the LC connection kit. This LC connection kit contains tubing for standard-bore LC only and is not suitable for use in micro LC applications.

1. In the LC connection kit a tubing cutter (p/n 250.102) is supplied to cut the supplied tubing to the appropriate length. Take care when making tubing connections in the flow path between injector and cell. Keep tubing length between injector - column cell to a minimum. Make sure to make a straight cut and that the tubing ends are properly inserted into the ports of the autosampler, column or cell when fixing the connector to avoid dispersion. The tubing end should touch the bottom of the port to achieve a zero-dead-volume connection.
2. The piston wash tubing is not part of the LC connection kit, it can be found in the P6.1L shipkit. Read instruction in manual p/n 194.0010 how to install. Also install the supplied drainage system (funnels, hoses, nozzles) for leak management as described in the pump user manual.
3. The tubing between pump purge valve and pulse damper is not part of the LC connection kit. This part can be found in the pulse damper shipkit. Follow the LC connection kit install guide (p/n. 180.7001W) for instructions concerning the connection between pump head and pulse damper (paragraph 'Instructions for connecting the flexible 1/32" OD tubing with fused 1/16" end sleeves'). The pulse damper, p/n 250.EZZ00NB has to be mounted in a bracket on the side of the P6.1 L pump using the part and instructions supplied in the shipping box of the damper.
4. The P6.1L pump with integrated degasser comes with pre-installed tubing between degasser and pump inlet. Reordering information for a replacement tubing is: Degasser outlet assembly, P6.1 (p/n 180.0206B).
5. For optimal performance it is required to passivate all metal parts in this system using a 15% solution of HNO<sub>3</sub>. See LC connection kit install guide for instructions.
6. For connections with a legacy VT-03 flow cell instead of SenCell use fingertights from the VT-03 ship kit: 250.1575 Fingertight M5.
7. When installing the filter, push the tubing deep into the port that is connected to the bottom inlet until it holds. Replacement filters can be ordered as '*PEEK filter for 1/8" MP inlet, 2um*' (pn. 250.1704).

### Legend LC tubing\*

- FEP 1/8", 1.59 mm ID, transparent
- PEEK 1/16", 0.50 mm ID, orange-striped
- PEEK 1/16", 0.25 mm ID, blue-striped
- PEEK 1/16", 0.13 mm ID, red-striped
- PEEK 1/16", 0.064 mm ID, pink-striped
- Silicone 3 mm, 1 mm ID, transparent
- Stainless Steel 1/16", 0.50 mm ID, metal

\*) Note that the color coding of the LC tubing in the drawing does not necessarily reflect the real color of the corresponding tubing.